


Detection of Avian Influenza H5-Specific Antibodies by Chemiluminescent Assays

Appendix

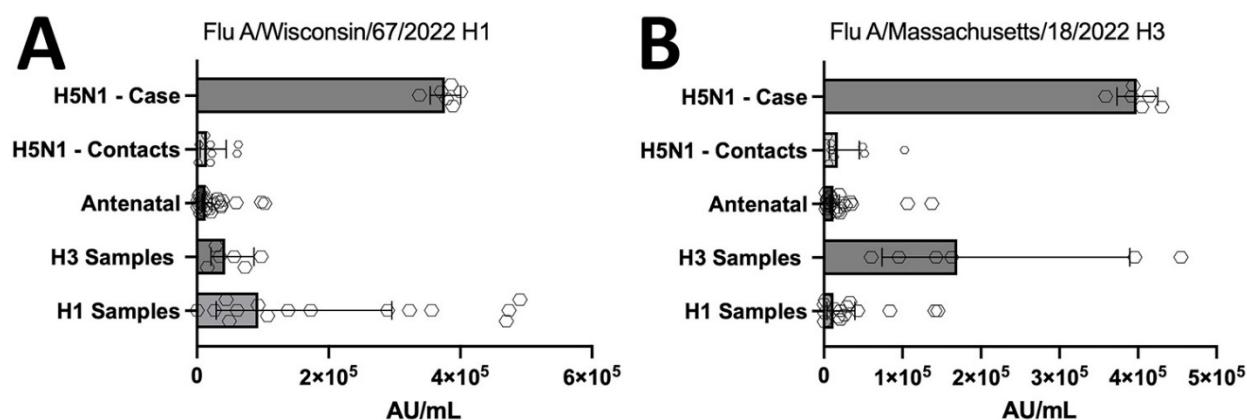

Appendix Figure. Antibodies in human samples from an individual infected with H5N1 shows cross-reactivity with H3 and H1 antigens. A) Human serum samples were tested using the MSD V-Plex Respiratory Panel 7 (IgG) kit, diluted 1:5000 in the manufacturer-provided diluent.